

AES FILE OPERATION OPTION EmergencyStop(E,ESC)

OFF **SCAN** HALT ABORT

LIA Signal = 0.000E-03 mV

Scan Params


Control Panel

SAVE AS 0771.AES

Load Spectrum

Anal. Window

LOADED from E:\CMAホームページ用データ\0174.AES - 2006-09-28 12:12:42

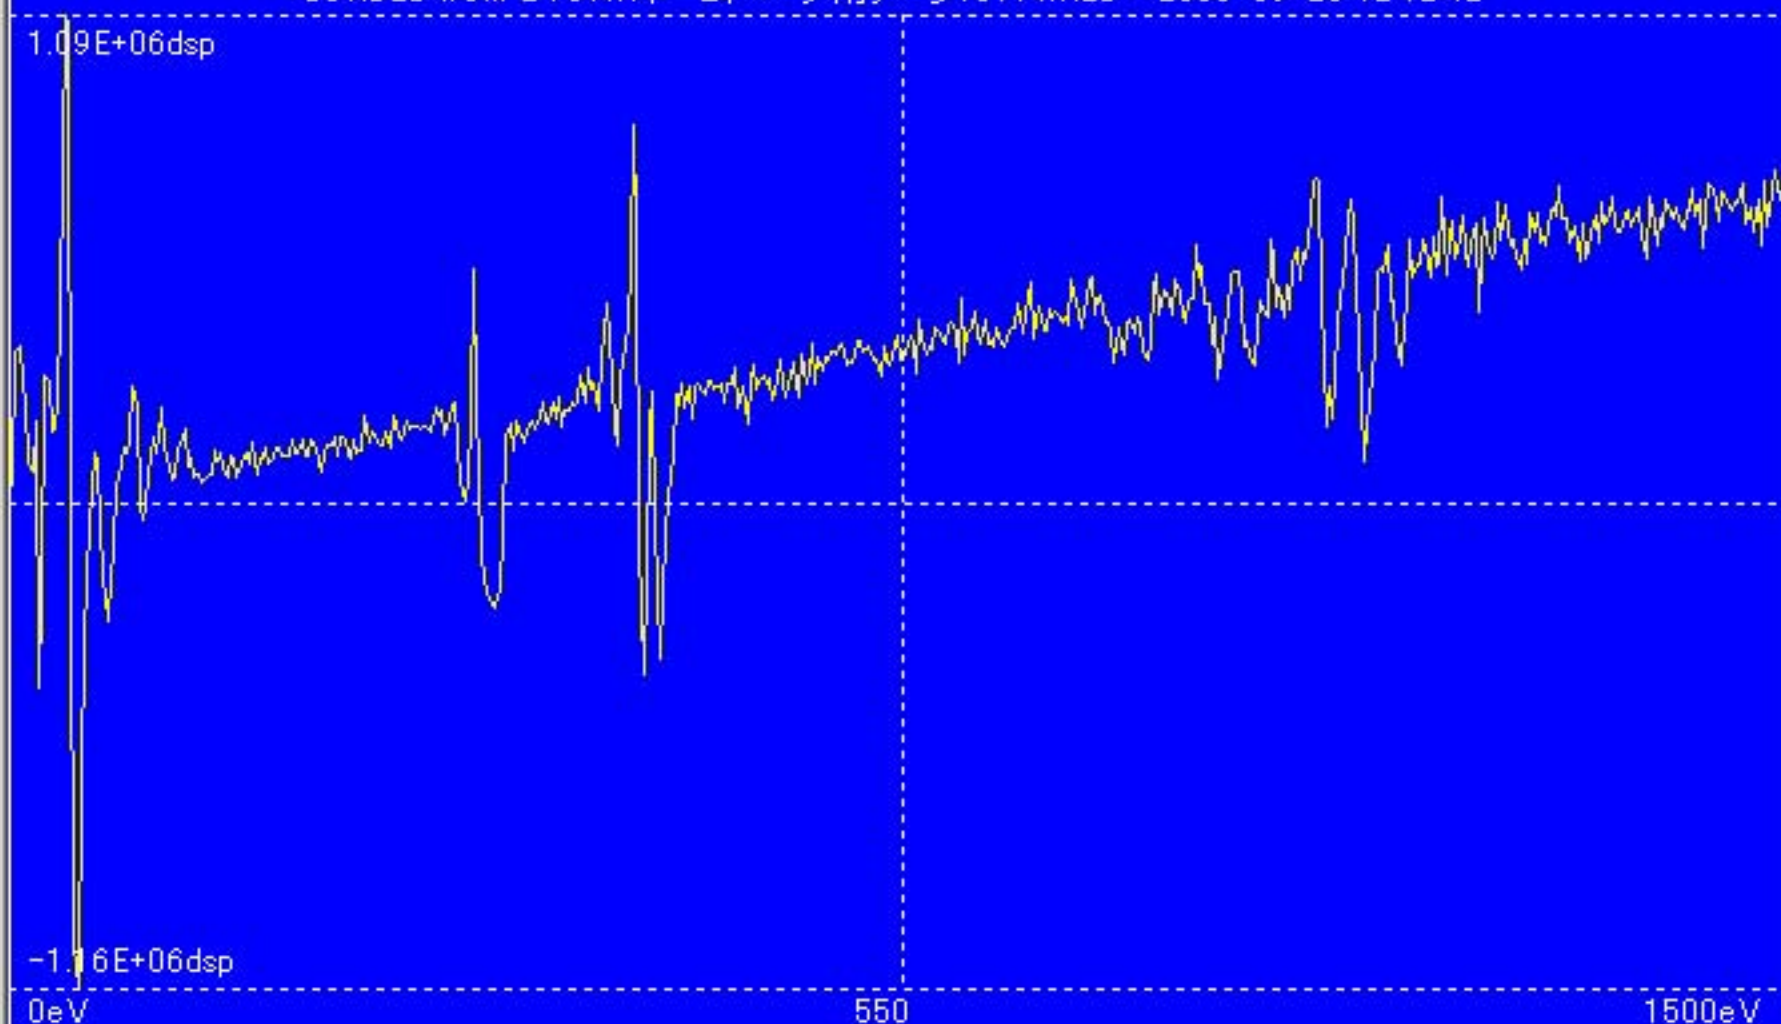

Lock-In E Gun



Filament

0.08 A

Emission

0.02 mA

Samp Curr

-44.26 uA

E Gun E0

-8 eV

CMA E

-9.6 eV

MULT

0.00 kV

ALL OFF

PRM: K.E.=323eV (level =+4.39E+06 dsp): Rh(MNN:307eV)

Kitano Seiki Co., Ltd.